


ANALYZER SOLUTIONS FOR YOUR PROCESS!

Model 304 Moisture in Chlorine Analyzer (MCA)

Chlorine manufacturers know the importance of measuring moisture in chlorine. Chlorine is formed by the electrolysis of brine, therefore chlorine is wet when produced and must be dried before compression and liquefaction. When dried chlorine comes in contact with water, hydrochloric acid is formed, causing corrosion to proceed rapidly in compressors and plant piping, which must be protected. The AMETEK Model 304 Moisture in Chlorine Analyzer (MCA) offers a solution to the problem of making an accurate, repeatable and reliable measurement of moisture in dried chlorine gas.

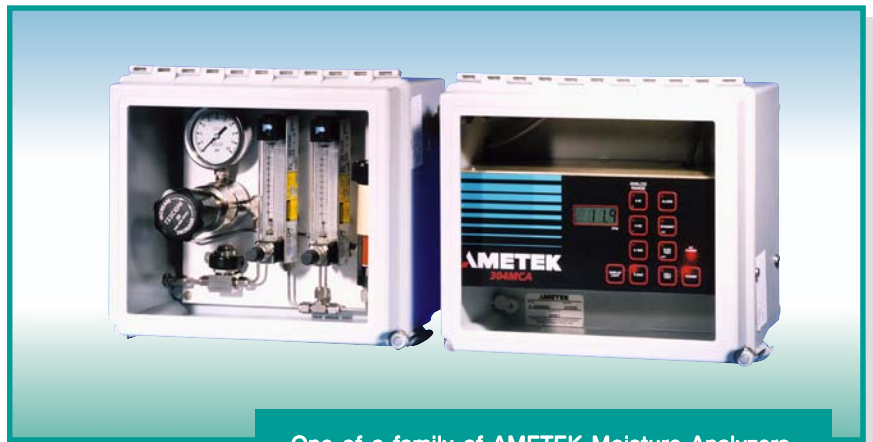

One of a family of AMETEK Moisture Analyzers

SUPERIOR BENEFITS

Two Polyester 4X Enclosures

The Model 304MCA consists of two polyester NEMA 4X enclosures. One enclosure houses the sample system and sensor, and the other contains the electronic controller/display. This separation protects the electronics, preventing damage should a leak occur in the sample system. Being mounted in a NEMA 4X enclosure permits the sample system to be installed close to the sample tap for fast and accurate measurement.

Materials of Construction

The Model 304MCA's sample-wetted materials are P₂O₅, Monel, Teflon, fluorocarbon resin, Kynar, glass, platinum, and Viton, making the analyzer resistant to attack by chlorine. The result is high reliability and minimal maintenance.

True Process Analyzer Features

The 304MCA is the moisture analyzer of choice for accurately measuring moisture in chlorine. A 4-20mA output compatible with a 625-ohm maximum load, transmits the moisture level to a recorder or control center. A built-in bypass flowmeter

increases total sample flow to keep response time to a minimum. The 304MCA is equipped with a digital moisture indicating meter, all solid state electronics, a rugged plug-in moisture cell, particulate filter, easily replaceable pressure regulator and Cl₂ calibrated flowmeter.

Electrolytic Cell

The electrolytic cell is in a self-contained cartridge that can be replaced in seconds. It does not require calibration, and is virtually specific to water. Sample connections are made automatically when the cell is inserted. Electrical connections are made through wires and a two-pin plug.

After-Sale Support

Our AMETEK Service Assistance Program is available to all AMETEK analyzer customers. ASAP is a comprehensive package of after-sale support programs, from hands-on training, to 24-hour phone help, to warranty extension. Contact AMETEK for additional details. (ASAP programs may have limited availability in some world areas.)

PERFORMANCE SPECIFICATIONS

Range: 0 to 1000 ppmv (0 to 2000 ppmv range possible with reduced sample flow)

Sensitivity: 1.0 ppmv

Accuracy¹: 2 ppm or $\pm 20\%$ of the display reading, whichever is greater

Sample Pressure and Flow Requirements²: Pressure: Vacuum to Max 2758 kPa (400 psig); Flow Rate: 100 mL/min plus bypass

Utility Requirements: 100 to 130 VAC or 200 to 260 VAC (specify required power when ordering), 10 W maximum

Analog Output: 4-20 mA DC proportional to range selected, compatible with 625-ohm maximum load

Alarms: Rated for 1 A, 24V DC, normally open and normally closed contacts; user-settable to fail-safe or low-power operation

Ambient Temperatures²: 0 to 40°C (32 to 104°F)

External Connectors: Gas IN and OUT fittings for 1/8-inch OD tubing. Internal connections for analog output and alarms; relay jumper changes operation to fail-safe mode

Front Panel Controls: Analog Ranges 0 to 10, 100, 1000 and 2000 ppmv

- Display light
- Alarm
- Standby power
- Electrical test
- Cell test
- Power

Cabinet Weights: Sample 9.1 kg (20 lb.), Electronics 5.6 kg (15 lb.) (each)


Cabinet Dimensions (W x H x D): 61 x 31.8 x 15.9 cm (24 x 12.5 x 6.25 in.)

Approvals and Certifications

- UL/CSA General Safety Requirements
- UL/CSA Class I, Division 2, Groups A, B, C, D T4A
- Complies with all relevant European directives

1. Consists of flowmeter accuracy plus analytical accuracy.

VAPOR PRESSURE OF CHLORINE

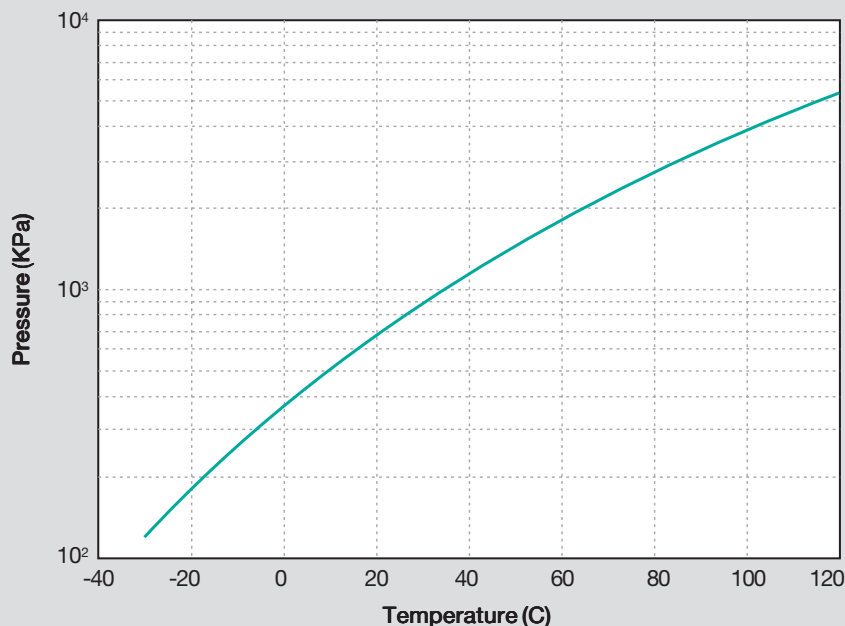

²The AMETEK Model 304MCA is a gas-phase analyzer. It is the customer's responsibility to ensure that liquid chlorine is not introduced into the 304MCA. The chart shows the vapor pressure curve of chlorine.

Equation: Vapor Pressure in pascals (Pa), T in kelvins

$$= \exp(71.359 - 3855.6/T - 8.5216 \ln T + 0.012386T)$$

Source

Calculated from Equation In:

Daubert, T.E., and Danner, R. P., Physical and Thermodynamic Properties of Pure Chemicals, Hemisphere Publishing Corporation, Washington, Philadelphia, London, 1992

One of a family of innovative process analyzer solutions from AMETEK Process Instruments. Specifications subject to change without notice.

USA - Pennsylvania
150 Freeport Road
Pittsburgh, PA 15238
Ph. 412-828-9040
Fax 412-826-0399

MANUFACTURING LOCATIONS



CANADA
2876 Sunridge Way N.E.
Calgary, AB T1Y 7H9
Ph. 403-235-8400
Fax 403-248-3550

USA - Delaware
455 Corporate Blvd.
Newark, DE 19702
Ph. 302-456-4400
Fax 302-456-4444

USA - Oklahoma
2001 N. Indianwood Ave.
Broken Arrow, OK 74012
Ph. 918-250-7200
Fax 918-459-0165

AMETEK
PROCESS INSTRUMENTS
www.amtekpi.com
© 2004, by AMETEK, Inc. All rights reserved.
304MCA (12/09/04)



SUPPORT LOCATIONS

USA - Texas
Ph. 281-463-2820
Fax 281-463-2701

CHINA - Beijing
Ph. 86-10-85262111
Fax 86-10-85262141

CHINA - Shanghai
Ph. 8621 6426 7049
Fax 8621 6426 7054

FRANCE
Ph. 33 1 30 68 69 20
Fax 33 1 30 68 69 29

GERMANY
Ph. 49 21 59 91 36 0
Fax 49 21 59 91 36 80

MIDDLE EAST - Dubai
Ph. 971-4-881 2052
Fax 971-4-881 2053

SINGAPORE
Ph. 65-6484-2388
Fax 65-6481-6588